This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS

- TEXT CUT OFF AT TOP, BOTTOM OR SIDES

- FADED TEXT

- ILLEGIBLE TEXT

- SKEWED/SLANTED IMAGES

- COLORED PHOTOS

- BLACK OR VERY BLACK AND WHITE DARK PHOTOS

- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

As rescanning documents *will not* correct images,
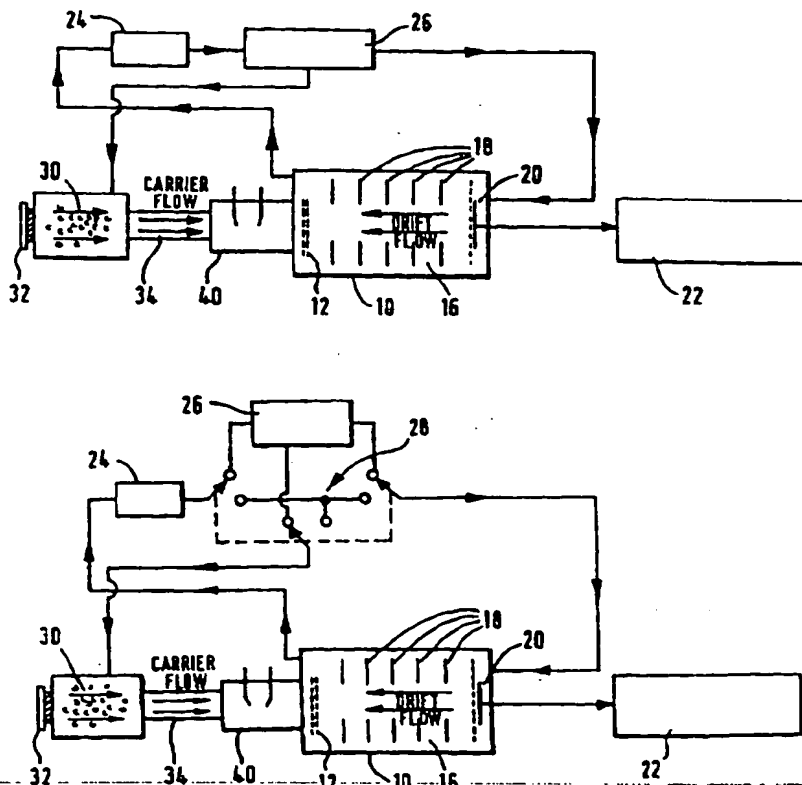please do not report the images to the
Image Problem Mailbox.

PCT

INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification 6 : G01N 27/64	A1	(11) International Publication Number: WO 97/28444 (43) International Publication Date: 7 August 1997 (07.08.97)

(54) Title: CORONA DISCHARGE ION SOURCE FOR ANALYTICAL INSTRUMENTS

(57) Abstract

An ion mobility spectrometer comprises an ion mobility cell (10) into which molecules of a sample to be analysed are introduced. The ion mobility cell (10) is doped with ions produced by a corona discharge ionisation source (40). In one mode of operation, the corona discharge ionisation source (40) operates to produce a continual dopant stream, and in a second mode of operation, the corona discharge ionisation source (40) produces dopant ions selectively. In the non-continuous mode of operation, the ion mobility cell (10) may be doped with chemical dopant ions instead, switching between the two dopant regimes being accomplished very rapidly. The ion mobility spectrometer is particularly suitable for the detection of explosive compounds and narcotics, the ion mobility spectrum of explosives doped with ions from the corona discharge ionisation source differing from the ion mobility spectrum of such explosive compounds doped with chemical dopants.

CORONA DISCHARGE ION SOURCE FOR ANALYTICAL INSTRUMENTS

The present invention relates to a corona discharge ion source for use in analytical instruments, and in
5   particular for use in ion mobility spectrometers.

Hitherto, corona discharge sources have been used in ion mobility spectrometers in order to produce the primary ions required for the operation of the instrument.
10   Device is shown in co-pending published PCT application No. WO/9311554.

The principle reason for employing such corona discharge ion sources has been to replace the most frequently used
15   nickel 63 radioactive ionisation source. The corona discharge ion source is significantly cheaper than the nickel 63 source. It is also not subject to the health and safety requirements of a radioactive source and may therefore be more readily transported across borders and
20   so forth.

In substituting a corona ion source for the nickel 63 source, the emphasis has been to replicate as far as possible the ion-molecule chemistry produced by the
25   nickel 63 source, in order to ensure that an ion mobility spectrometer fitted with a corona discharge ionisation source detects the same range of compounds as when fitted with a nickel 63 source.

30   Figure 4 shows a typical output of an ion mobility spectrometer in the absence of an introduced compound or impurity to be detected. This peak corresponds to stable molecular ion species which have resulted from a complex series of ion-molecule reactions and is referred to
35   generally as the Reactant Ion Peak (RIP). When a sample

to be detected, such as in this example RDX (a major constituent of Semtex), is introduced into the ion mobility spectrometer, a further peak (or peaks) is detected as well as the reactant ion. The problem with
5   this procedure is that, in practice, the sample entering the ion mobility spectrometer contains a significant number of other compounds. If these have a similar mobility to the RDX ions, the signature peak of the RDX is reduced in amplitude and may in certain cases be
10   suppressed by the contaminants to such an extent that the RDX peak is no longer clearly visible. A schematic plot of the output of an ion mobility spectrometer under these conditions is shown in Figure 11.

15   A technique known as chemical doping has been developed to address this problem, and is frequently used in ion mobility spectrometry and chemical ionisation mass spectrometry. Chemical doping may be used irrespective of the ionisation source used to generate the primary
20   ions (i.e. either a corona discharge ion source or a nickel 63 ion source) to change the way in which sample vapour introduced to the device becomes ionised.

The use of such chemical dopants is described in
25   Analytical Chemistry, 56(11):1794-1797 by Procter and Todd.

In outline, a chemical dopant, typically in the form of a vapour or gas is introduced into the ionisation region
30   of the instrument such that the dopant chemical becomes the dominant reactant ion species in the ionisation region of the instrument and, if an incoming sample vapour molecule is to be ionised, it must undergo an ion-molecule reaction with the dopant reactant ion.
35

According to the present invention, there is provided an analytical instrument including a corona discharge ionisation source arranged to generate corona dopant ions.

When the energy density around the point of a corona discharge is above a certain level, new reaction compounds may be generated. Typically, when the discharge is conducted in air, these compounds will include ozone, oxides of nitrogen and excited neutral states of nitrogen. Since these reaction compounds influence the ion-molecule chemistry in an analytical instrument, previous work has been directed towards minimising the concentration of the compounds, so that their effect on the functioning of the instrument is negligible.

It has been found, however, that the products of the corona discharge ionisation source may be employed as dopant ions, whereby the ion-molecule chemistry of the instrument may be altered under external control.

Preferably, the analytical instrument is an ion mobility spectrometer, the ionisation region of which is doped by the corona dopant ions generated by the corona discharge ionisation source.

By means of, for example, electronic control of the corona discharge, the doping regime of an ion mobility spectrometer may be rapidly and easily altered to provide changing ionisation chemistry conditions, thereby to modify instrument sensitivity and/or selectivity readily.

Preferably, the corona discharge ionisation source is arranged to generate the corona dopant ions substantially

4

continuously. Under such conditions, only a few types of
sample vapours, such as explosive compound vapours, are
capable of efficient ionisation and hence detection.
Thus, the selectivity of the analytical instrument to
5   these compounds is better than that of a system undoped
by discharge compounds.

Alternatively, the analytical instrument may have
switching means for switching the corona discharge
10   ionisation source such that the dopant ions are generated
selectively. Thus, the analytical instrument fitted with
a corona discharge ionisation source can, at times,
operate under conditions such as to produce the corona
dopant ions to dope an ionisation region thereof, and
15   can, at other times, operate under conditions such as not
to produce those corona dopant ions, the instrument then
operating as an undoped system.

The change between a doped system and an undoped system
20   can be accomplished by electronic switching means, for
example, within a very short time, typically within a
fraction of a second. Thus a sample vapour administered
to the ion mobility spectrometer, for example, could be
quickly analysed under two different doping regimes.
25

Analysis of the sample vapour under the two different
regimes provides additional identification information.
For instance, the sample vapour may be ionised when the
system is undoped, but not when it is doped by the
30   discharge compounds, and this may help to indicate that
the sample vapour is not that from an explosive compound.
In another case, the mobility of the detected ion may be
different under the two doping regimes, and indicate that
the ion species formed from the sample vapour is
35   different in the two regimes. This has also provided

further discriminatory information, provided that all
sample vapours ionised in both regimes did not change
their mobility by the same amount.

5   Preferably, the analytical instrument further comprises
chemical dopant means arranged to generate different,
chemical dopant ions. Preferably the chemical dopant
ions are produced when the corona dopant ions are not
being produced by the corona discharge ionisation source.
10   The chemical dopant means may be a gas permeable source
fitted within a circulating gas flow of the analytical
instrument.

This mode of operation can be of value, for example, if
15   the electron or proton affinity of the corona dopant ions
produced by the corona discharge ionisation source are
greater than those of the chemical dopant ions available
from the permeation source.

20   If the analytical instrument is an ion mobility
spectrometer, then the primary ions necessary for
ionisation of a sample to be analysed may either be
generated by the corona discharge ionisation source which
also generates the corona dopant ions, or alternatively
25   may be generated by a radioactive source, such as nickel
63. In the latter case, the corona discharge ionisation
source may not be fitted in the ionisation region of the
instrument but instead external to that region, and
possibly outside the body of the ion mobility
30   spectrometer, for instance in a gas flow into the
instrument. For example, the corona discharge ionisation
source may be located in series with an incoming gas flow
associated with the cell.

35   Corona dopant ions generated by the corona discharge

would be carried into the cell and act as dopants in the manner described above, without the corona discharge source acting as the means of ionisation of the incoming sample.   This method may enable the provision of a high
5   concentration of corona dopant ion into the instrument to more positively dope the cell.   Generation of the corona dopant compounds may be controlled electronically to achieve added instrument sensitivity and selectivity.

10   The corona discharge ionisation source is preferably a pulsed corona ioniser with either a single or a double point source.

15   In order that the invention may be more readily understood a specific embodiment will be described by way of example only, with reference to the accompanying drawings in which:

20   Figure 1a is a diagrammatic representation of the essential elements of an ion mobility spectrometer used to demonstrate the operation of corona ion source doping, with constant chemical dopant supply;
                Figure 1b is the ion mobility spectrometer of Figure 1a, with a switching arrangement to permit selective
25   doping with the chemical dopant instead of a constant chemical dopant supply;
                Figure 2 is a schematic representation of the corona ionisation source employed in the apparatus of Figure 1;
30   Figures 3 and 4 are plots of ion peaks representative of the use, and non-use of corona ionisation source doping in the ion mobility spectrometer of Figure 1;
                Figures 5 to 10 inclusive are plots of ion peaks
35   obtained from the ion mobility spectrometer of

Figure 1, with the introduction of various samples, as described below, and

Figure 11 is a schematic diagram of the output of a prior art ion mobility spectrometer when undoped by chemicals.

Referring to Figures 1a or 1b, the apparatus used to demonstrate the occurrence and application of corona ion source doping comprises an ion mobility cell 10, having an ion injection gate 12, and a drift region 16, provided with electrodes 18 for establishing an electric drift field along the drift tube 16, and a collector electrode 20.

Sample material is introduced into the ion mobility cell 10 by way of the thermal desorption source 30, and corona ionisation source 40, attached to the ion mobility cell 10 in the region of the ion injection gate 12.

Material introduced into the thermal desorption source 30, by means of a sample wipe 32, is heated sufficiently to cause vapourisation, desorbed vapours being swept, by means of a carrier gas flow through tube 34 into corona ionisation source 40, where ionisation takes place, sample ions, together with any unreacted dopant ions, being swept into ion mobility cell 10, which is operated at a cell temperature of 105°C.

In the conditions pertaining to the plots obtained, the sample is offered to the system in particulate form upon

8

PTFE sample wipes 32. Thermal desorption source 30 provides a stream of dry air at 200°C directed onto the sample wipe 32 and thus releases analyte vapour into the carrier gas flow through tube 34. The analyte vapour is subsequently swept into the dual point corona discharge ionisation source 40 where, after a series of ion molecule reactions between analyte molecules and reactant ions formed in the source, product ions are formed. These product ions (and usually some unreacted reactant ions) are then gated into the drift region 16 of the cell where they are separated electrically according to their ionic mobilities and detected.

The ion mobility cell 10 is provided with ancillary means such as a pump 24, for establishing the usual carrier and drift gas flows necessary for its proper operation, together with means for establishing the necessary electric drift field by means of potentials applied to electrodes 18, all as well known in the art.

In Figure 1a, a chemical dopant source 26 is arranged in a circulating gas flow of the analytical instrument, circulation being carried out by means of the pump 24. The chemical dopant source is, for example, a gas permeable source.

Figure 1b shows a different arrangement to permit the chemical dopant to be added to the ion mobility spectrometer selectively. Switching means 28 is employed within the circulating gas flow. This may include, for example, a valve (not shown). The switch 28 allows the chemical dopant source to be brought into and out of the gas flow circuit, as shown in that Figure.

The essential features of the ioniser are shown in Figure 2. The corona ionisation source 40 comprises two fine gold wires, 42 and 44, both of 10μm diameter, spot-welded onto clean tinned copper wires, 46 and 48, located within electrically-insulating Fluorosint holders, 50 and 52. Both points emerge into the source region 54 which has a circular cross-section of diameter 8mm. During operation, the source block 56 is electrically grounded at all times.

The corona ionisation source 40 described is operated

10

in a pulsed mode thus producing a packet of ions for analysis in the associated ion mobility spectrometer. Ions formed by the source 40 drift towards a standard Bradbury-Nielsen ion gate 58 through which they are injected into the drift space of the ion mobility spectrometer in the normal manner.

The delay between the corona pulse applied to the primary corona point 42, and the gating pulse applied to the ion injection gate 58 is optimised to maximise transmission of ions into the drift space of the spectrometer, which, with the geometry and dimensions of the source 40, is in the range 1ms to 2ms.

To achieve satisfactory operation of source 40, both a standing dc voltage and a pulsed voltage are applied to the primary point 42, both of the same polarity as the ions to be generated, whereas the secondary point 44 is held at a dc voltage of opposite polarity to that of the primary point.

The ion-molecule chemistry prevailing in the corona ionisation source 40 of the spectrometer can be altered significantly by switching the secondary point voltage from below to above the threshold voltage required to initiate a self-sustaining dc corona discharge at the secondary point 44.

When the corona discharge at the secondary point 44 is not self-sustaining (i.e. it requires an influence from the primary point to operate) the ion chemistry is to all intents identical to that of an ion mobility spectrometer

employing a standard nickel 63 ionisation source, whereas
a different ion chemistry (referred to as "leading edge"
chemistry) is observed when a self-sustaining corona
discharge is established at the secondary point 44.

It is therefore a simple matter to alter the ion
chemistry prevailing in the source region 54 by effecting
a discrete change in the voltage applied to the secondary
point 44. This may be done, for example, using a switch
51 which may be software controlled.

To achieve stable operation in the corona ionisation
source 40, the d.c. voltage applied to primary point 42 was
set between -300V and -600V and the pulse amplitude between
-1.5kV and -2.5kV. The experimental conditions were
identical for all spectra shown in the accompanying figures
of the drawings, with the one exception that the secondary
point voltage was set at +800V when operated with normal
ion chemistry - with no self-sustained corona discharge on
point 44, and at +1100V when operated with "leading edge"
chemistry - with a self-sustained discharge on point 44.

The ion-molecule chemistry which prevails in the
ionisation region of an ion mobility spectrometer equipped
with the pulsed dual-point corona discharge ionisation
source 40 described above can be altered significantly by
suitable variations of the corona point voltages. Negative
ion mobility spectra have been recorded with the corona
system operating (a) in a regime where the system response
is similar to that of a conventional nickel 63 ionisation
source (normal ion chemistry), and (b) where the energy
density at either corona point is high enough to introduce

12

an additional ion species into the reaction region. When
the latter is the case, a strong ion peak 60 is observed on
the leading edge of the normal reactant ion peak 62 as can
be seen in Figure 3. Where such a situation applies, the
effect is referred to as "leading edge" chemistry.

Figure 4 shows the reactant ion peak 64 obtained with
normal ion chemistry.

Both spectra were recorded with a clean PTFE
sample wipe 32 introduced to the system of Figure 1, and
were averaged over eight ion gate pulses.

All spectra presented in the drawings were signal
averaged over eight individual spectra produced during the
eight respective ion gate pulses, using a Nicolet 4904
digital oscilloscope fed from the signal processing and
analysing circuitry attached to the collector electrode 20
of the ion mobility spectrometer 10, and stored on floppy
disk.

RDX, a high explosive, has been selected as a typical
demonstration compound, which shows the qualitative
differences in the spectra when "normal" and "leading edge"
ion chemistry is used.

A quantity of 9ng of RDX was deposited on a clean
sample wipe and offered to the system of Figure 1. With
normal ion chemistry prevailing, three strong product ion
peaks 70, 72 and 74 are observed at 9.76, 10.47 and 11.13ms
on the spectrum illustrated in Figure 5.

The effect of introducing leading edge chemistry is to
suppress the peaks at 9.76 and 10.47ms and to produce an

13

additional product ion peak 76 at 11.48 ms, as can be seen in Figure 6. This obvious change in the spectra could be utilised as an additional means of identification for RDX.

The spectra shown in Figures 5 and 6 were recorded for the same sample, as the sample wipe 32 was not removed from the thermal desorption source 30 between chemistry changes.

A clean sample wipe was wiped on a piece of paper which had been contaminated with "WD-40" lubricant and offered to the system of Figure 1.

Figure 7 shows the spectrum obtained with normal ion chemistry.

The effect of introducing leading edge chemistry is marked as seen in Figure 8. The wide peaks 80 and 82 at 14.5ms and 17.5ms are greatly reduced in intensity as are the peaks 84 at 10.5ms, and 86 between 7.0ms and 9ms. An additional peak 88, not apparent in the normal chemistry spectrum of figure 7, is observed at about 9.6ms.

The effect of a "WD-40" background on the response of the system to RDX, with both normal and leading-edge chemistry, is shown in Figure 9 and 10.

Figure 9 shows the spectrum which was obtained from a wipe which had been contaminated with WD-40 and also had 9ng of RDX deposited upon it. This spectrum was recorded with normal ion chemistry. Clearly, the three product ion peaks 90, 92, 94 associated with RDX vapour are observed as are the broad peaks 96 and 98 corresponding to WD-40 contamination.

However when the instrument of Figure 1 was operated

with leading edge chemistry, Figure 10 shows that the WD-40 contamination peaks 96 and 98 are suppressed in intensity but the RDX peaks 100, corresponding to the peaks 76 of Figure 6, persist, thus demonstrating the ability of the system of Figure 1, when used with ionisation source 40 in the leading-edge mode, to selectively suppress background contamination, without any significant loss in strength of the ion peaks 100 indicative of the presence of RDX.

Although the invention has been described with reference to an application in ion mobility spectrometry, the invention may also be applied in other appropriate instrumental applications where chemical doping has previously been employed.

In addition, the invention may be readily applied to the detection of narcotics which typically have a very high proton affinity. The chief difference in operation is that the ion mobility spectrometer must be operated in "positive ions" mode which is done by switching the polarity of the voltage at the discharge points. A suitably chemical dopant as an adjunct to the positive deportations produced by the corona discharge ionisation source is ammonia.

Other gases, such as Sarin gas, may also be detected.

CLAIMS

1.   An   analytical   instrument   including   a   corona
discharge ionisation source arranged to generate corona
5   dopant ions.

2.   An analytical instrument as claimed in claim 1, in
which the instrument is an ion mobility spectrometer, the
ionisation region of which is doped by the corona dopant
10   ions generated by the corona discharge ionisation source.

3.   An analytical instrument as claimed in claim 1 or
claim 2, in which the corona discharge ionisation source
is   arranged   to   generate   the   corona   dopant   ions
15   substantially continuously.

4.   An analytical instrument as claimed in claim 1 or
claim 2, further comprising switching means for switching
the corona discharge ionisation source such that the
20   corona dopant ions are generated selectively.

5.   An analytical instrument as claimed in claim 4,
further comprising chemical dopant means arranged to
generate different, chemical dopant ions.

25

6.   An analytical instrument as claimed in claim 5, in
which the chemical dopant means is a gas permeable source
fitted within a circulating gas flow of the analytical
instrument.

30

7.   An analytical instrument as claimed in any of claims
2 to 6, in which the corona discharge ionisation source
further generates the primary ions for ionisation of a
sample to be analysed.

35

16

8.   An analytical instrument as claimed in any one of claims 2 to 6, further comprising a radioactive source for generating the primary ions for ionisation of a sample to be analysed.

5

9.   An analytical instrument as claimed in claim 8, in which the corona discharge ionisation source is arranged outside the instrument.

10   10.   An analytical instrument as claimed in claim 9, in which the corona discharge ionisation source is arranged in a gas flow into the instrument.

11.   An analytical instrument as claimed in any one of
15   claims 2 to 10, in which the corona discharge ionisation source is a pulsed corona ioniser with a single point source.

12.   An analytical instrument as claimed in any one of
20   claims 2 to 10, in which the corona discharge ionisation source is a pulsed corona ioniser with a double point source.

13.   An analytical instrument as claimed in any one of
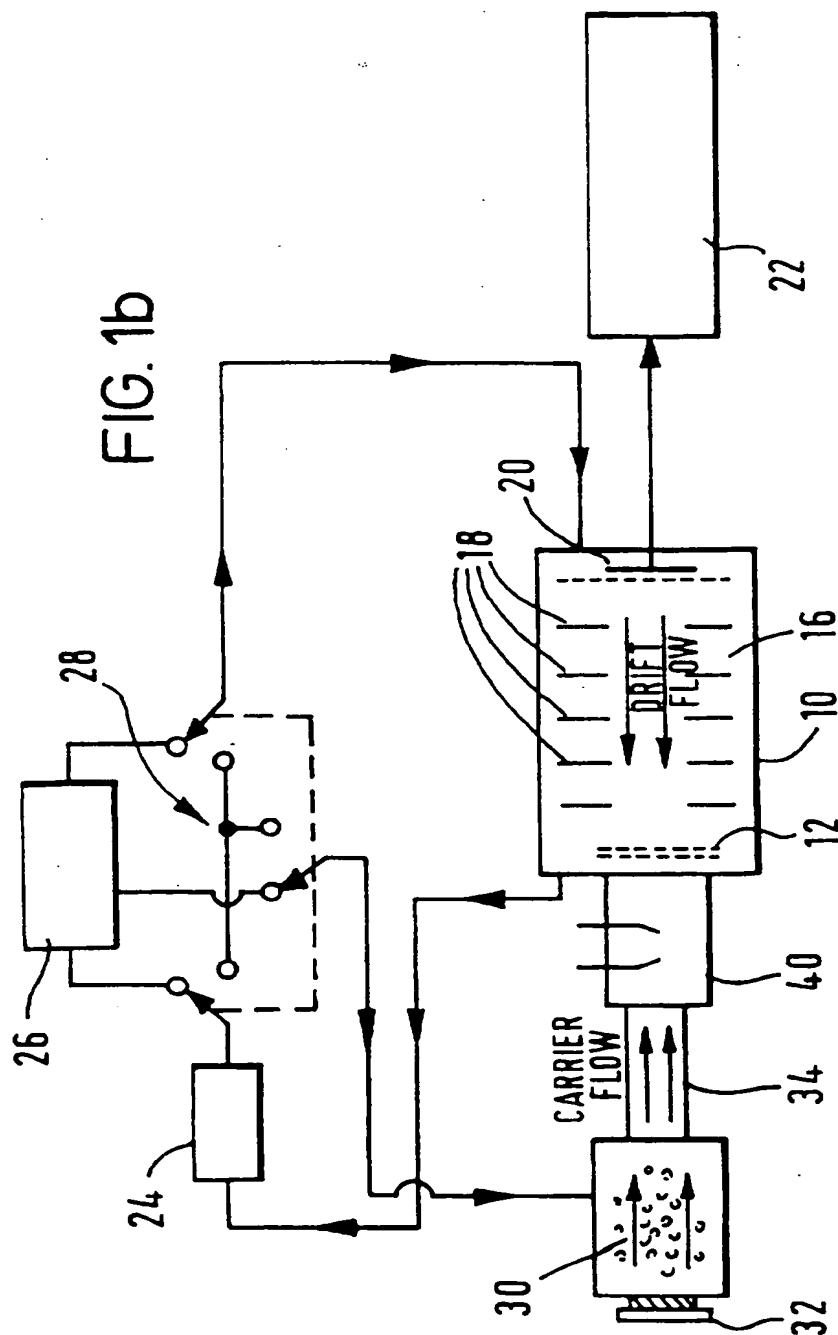25   the preceding claims, adapted to detect explosive compounds.

14.   An analytical instrument constructed and arranged substantially as specifically described with reference to
30   and as shown in Figures 1 to 10 of the accompanying drawings.
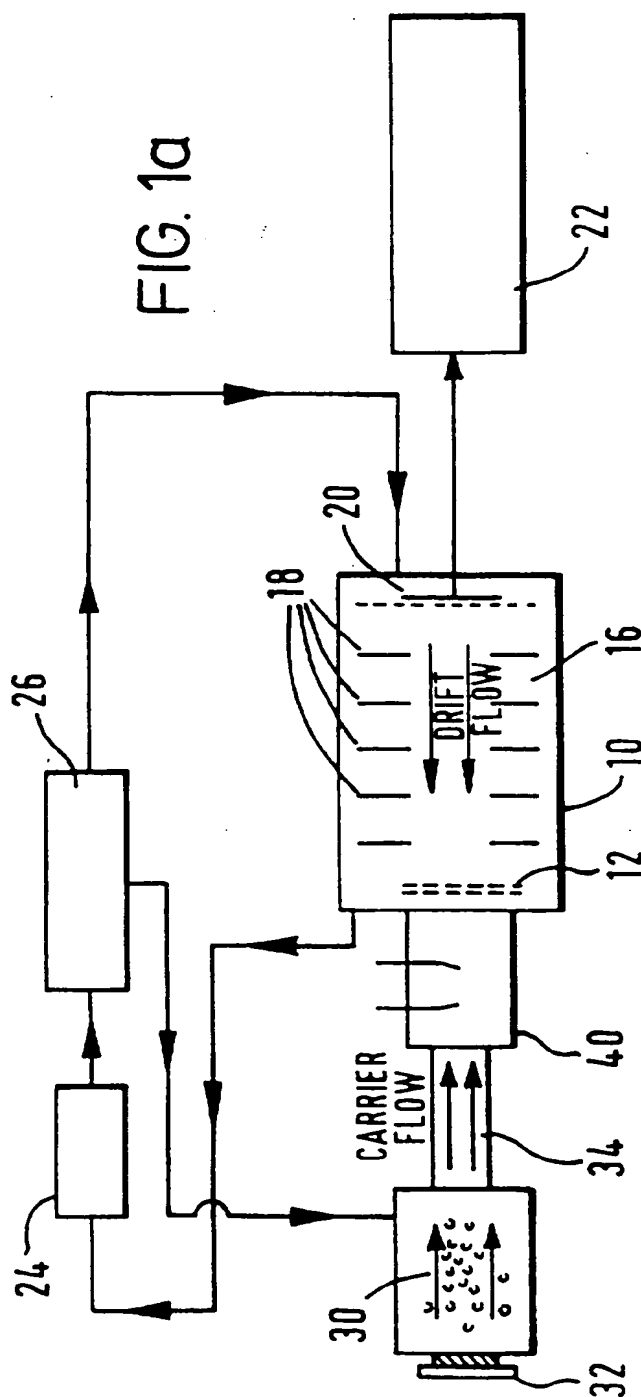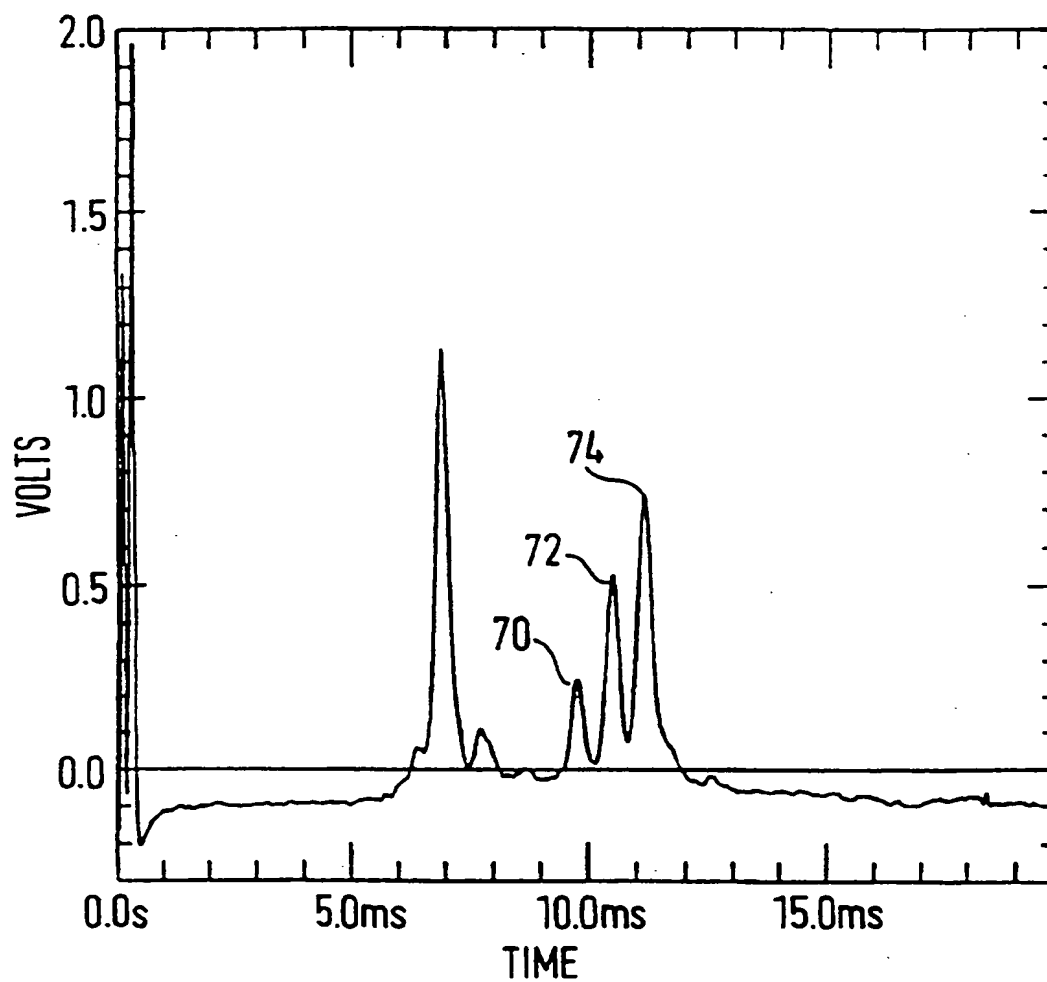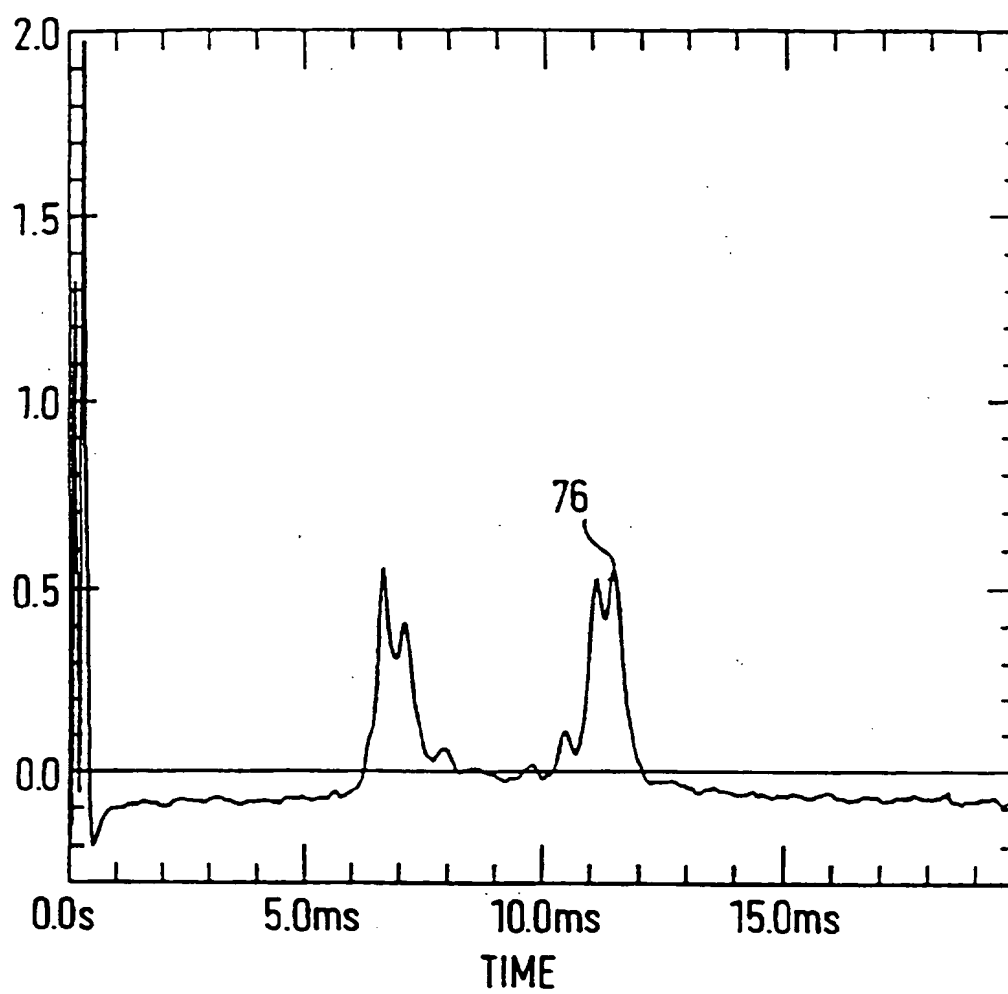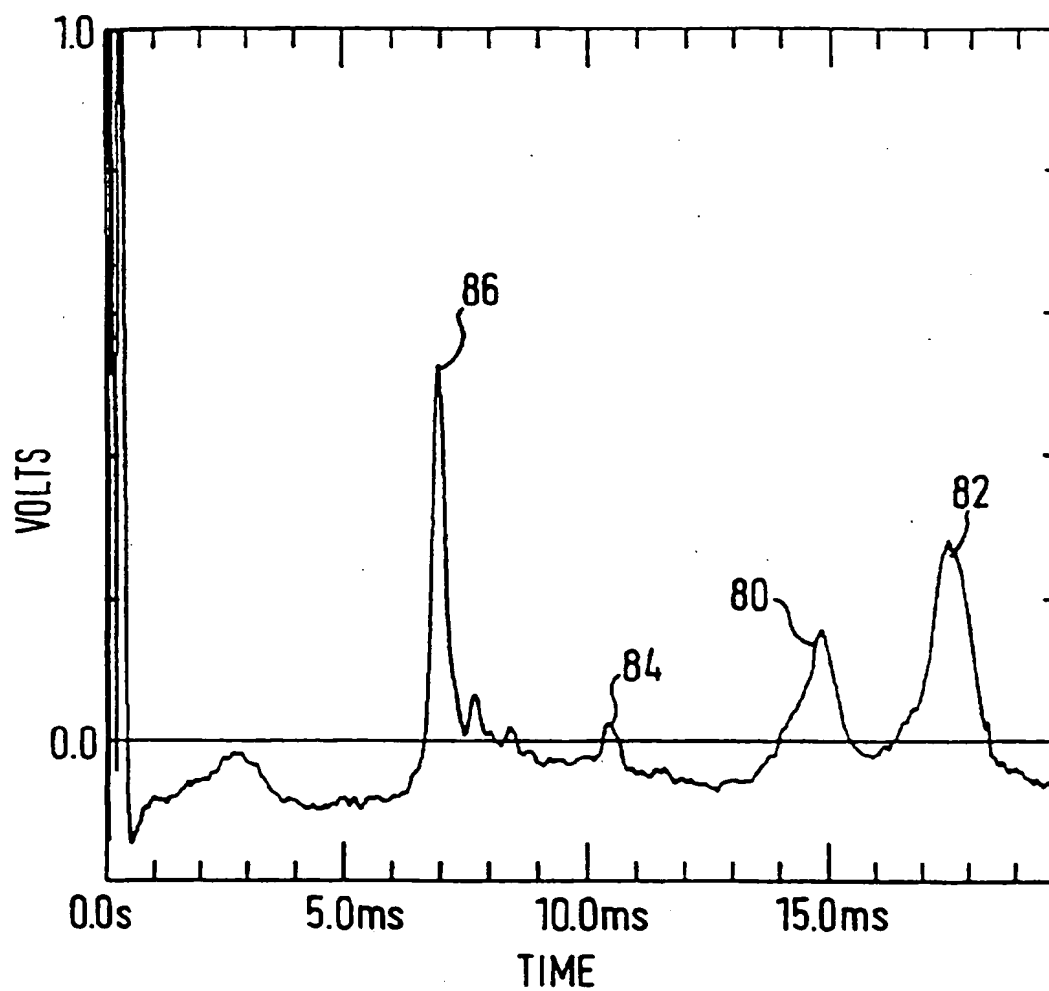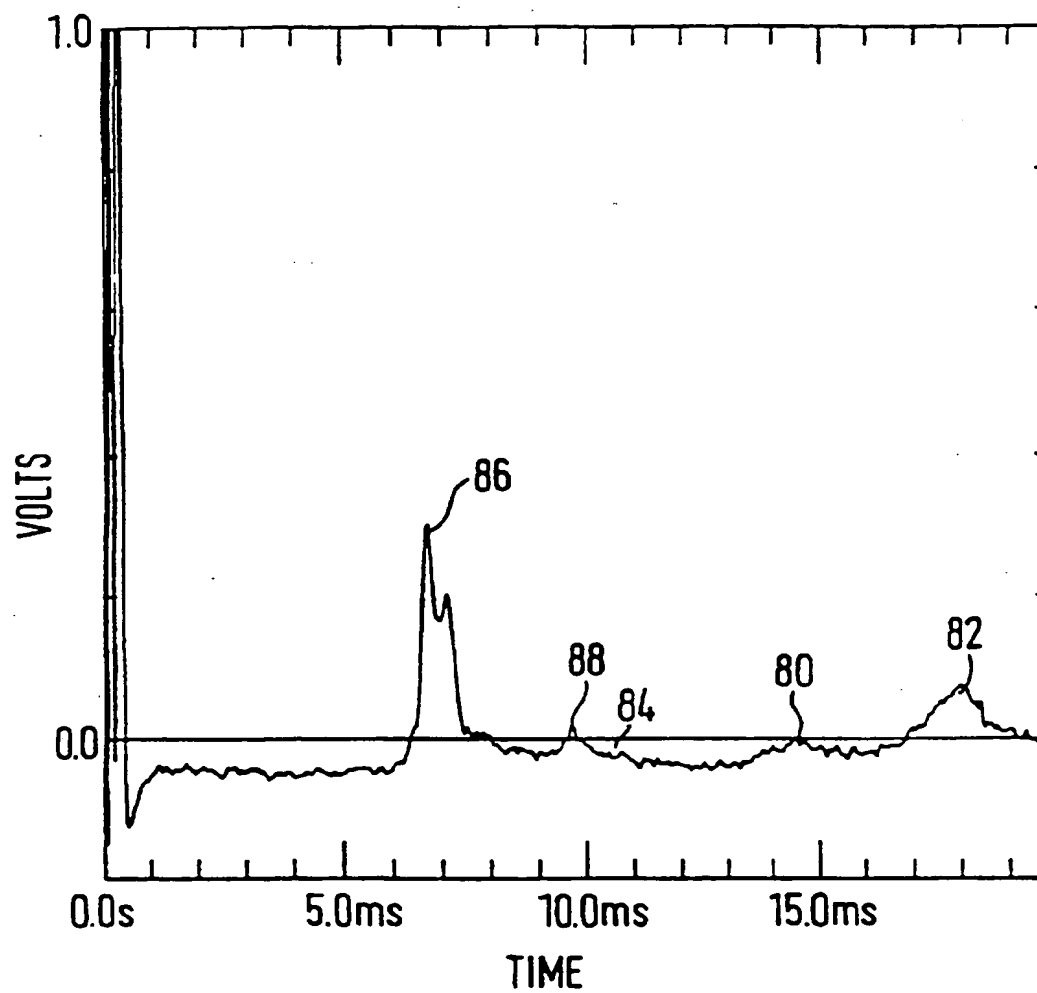
FIG. 1a
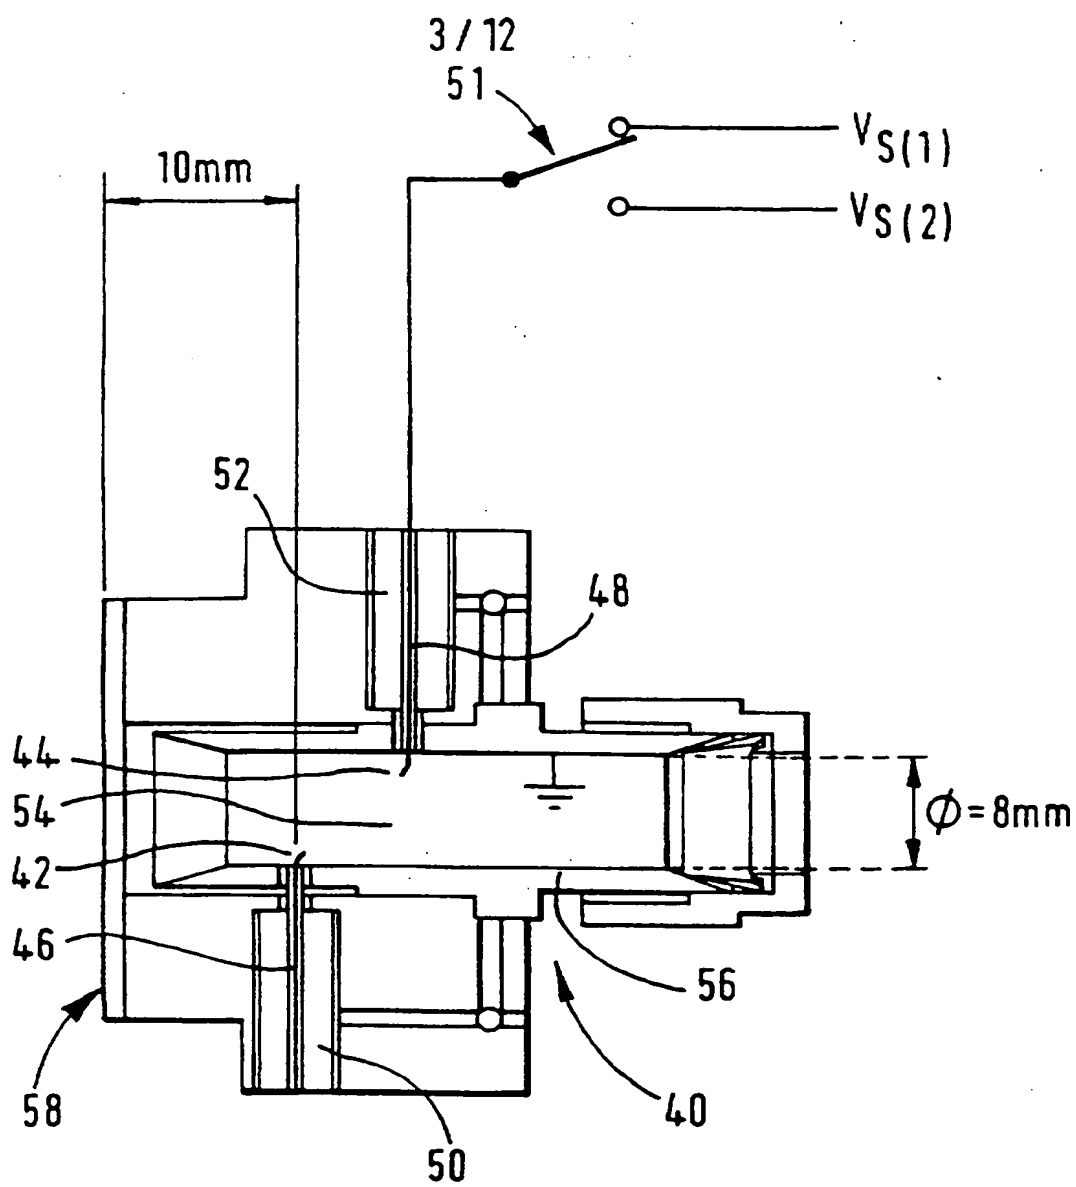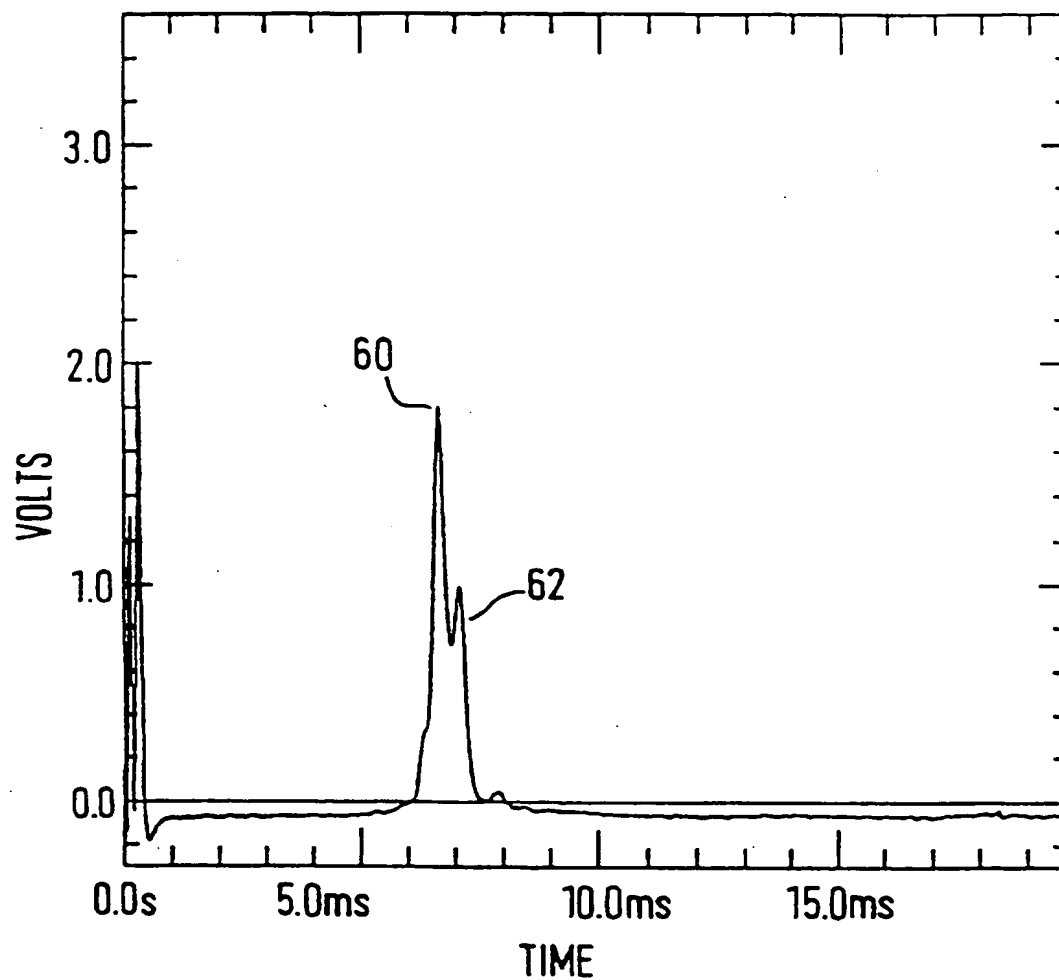
FIG. 1b

3 / 12

51

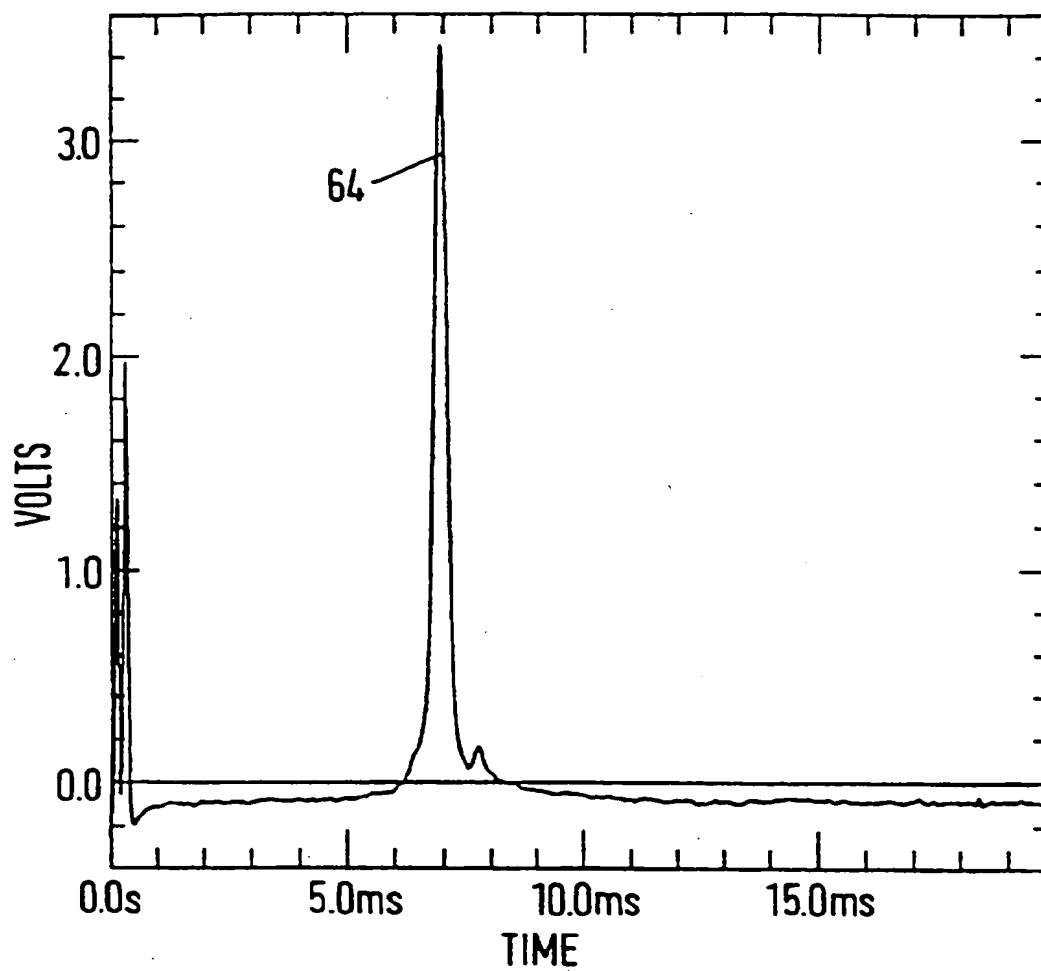$V_{S(1)}$

$V_{S(2)}$

10mm

52

48

44

54

42

46

58

50

56

40

$\phi = 8mm$

FIG. 2

FIG. 3

FIG. 4

FIG. 5

FIG. 6

FIG. 7

FIG. 8
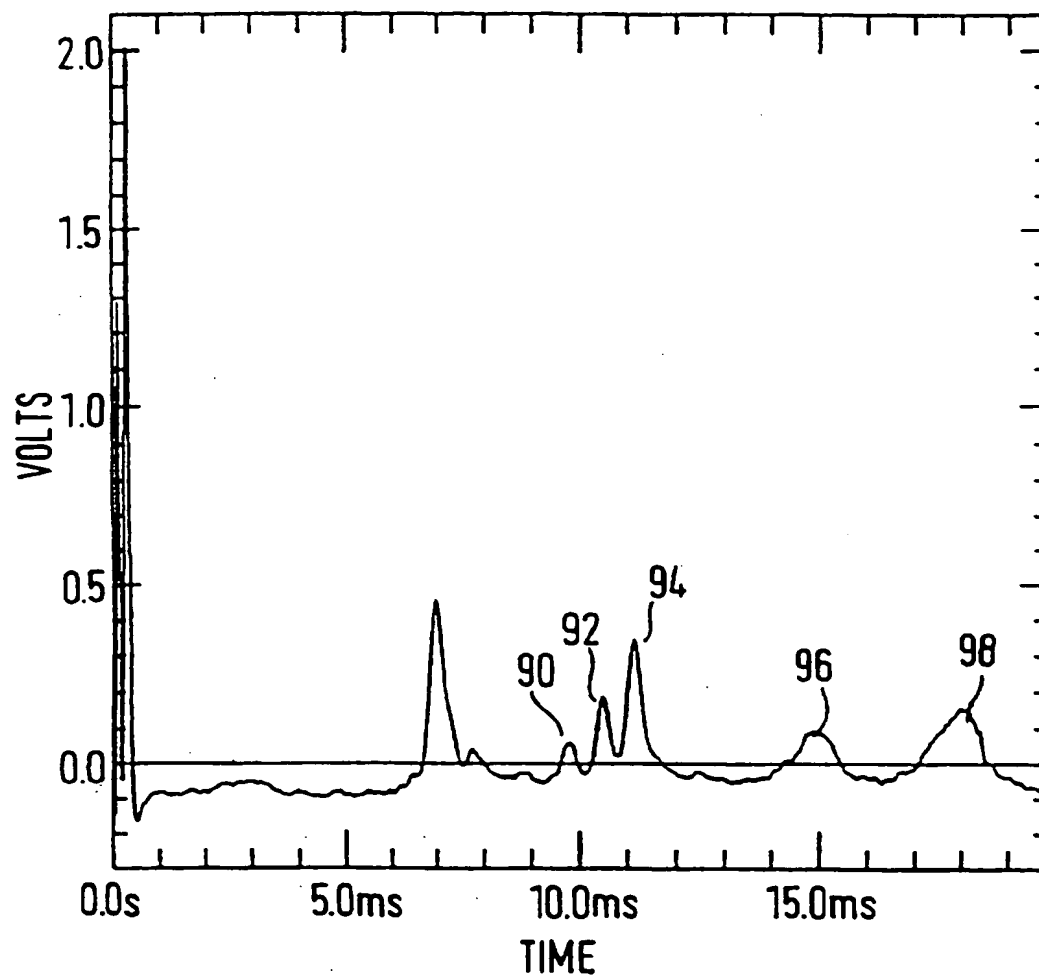
FIG. 9
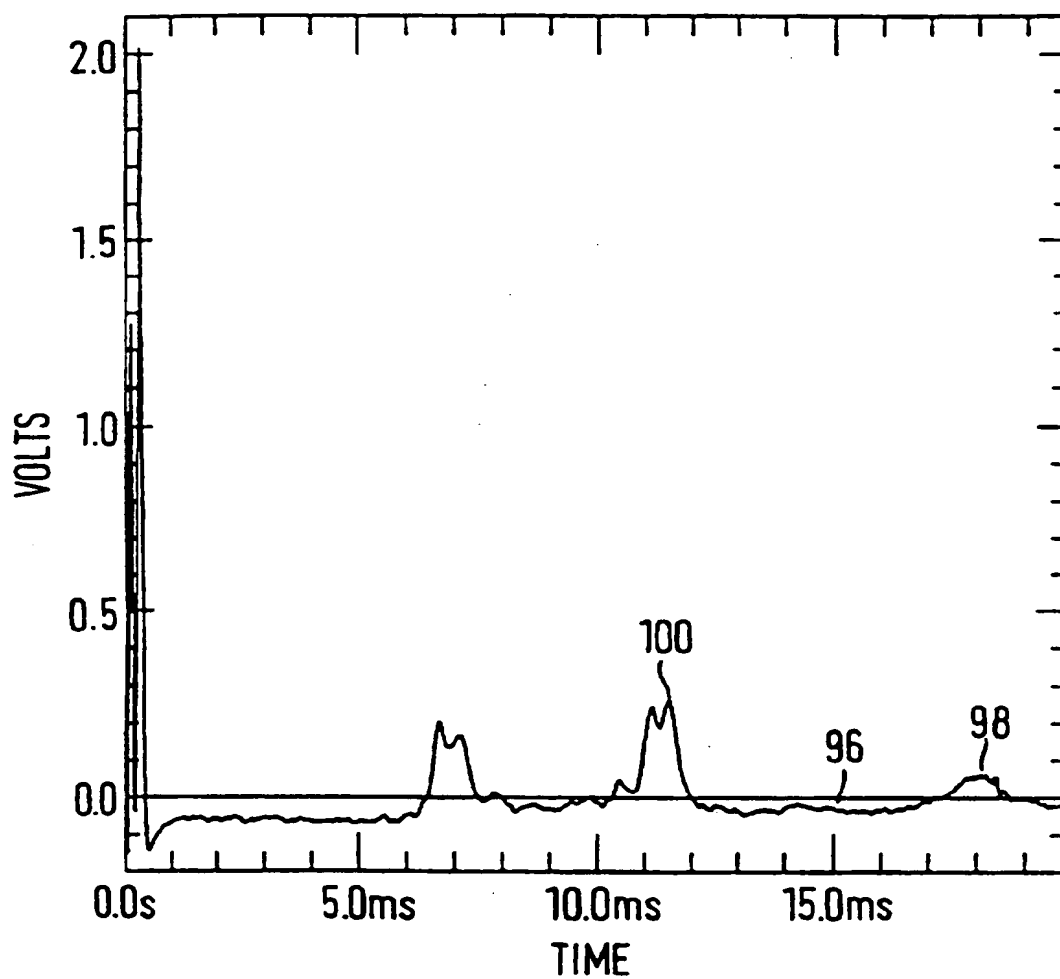
FIG. 10
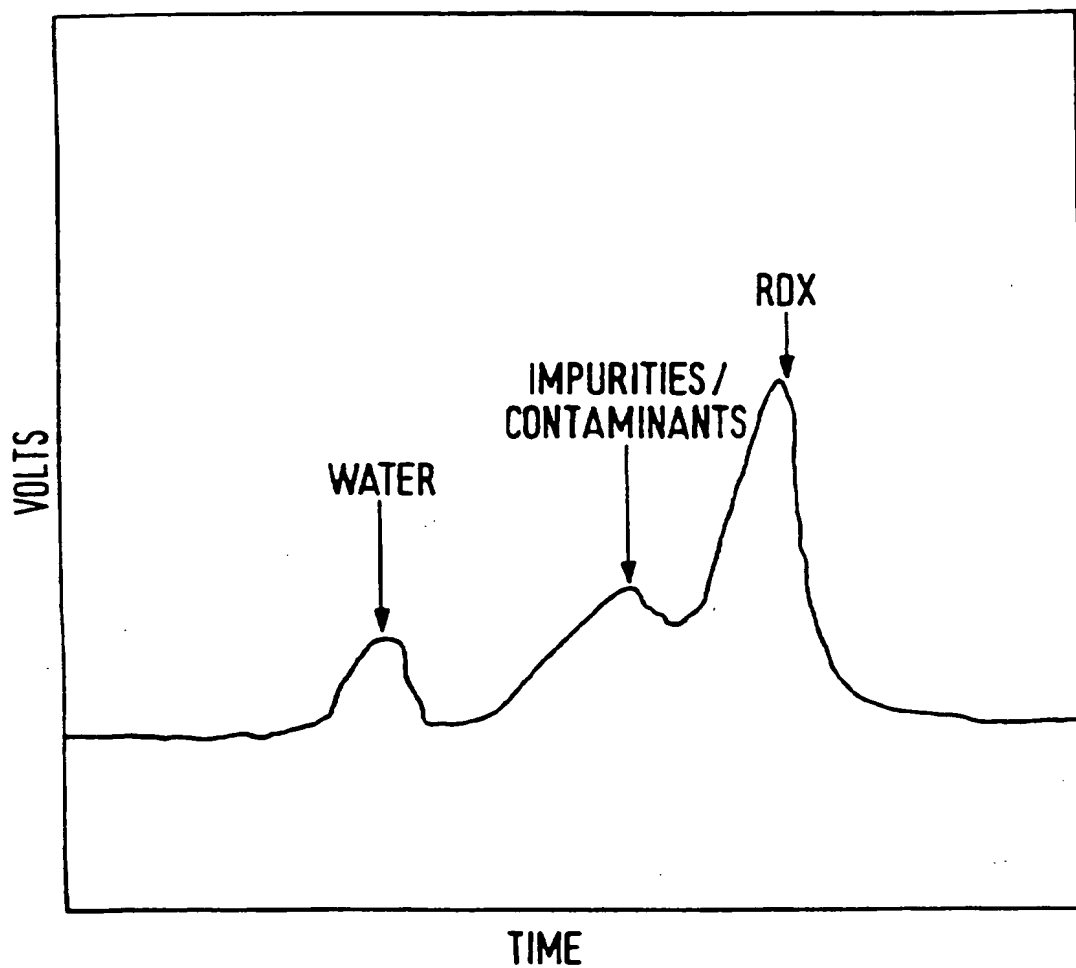
FIG. 11

A. CLASSIFICATION OF SUBJECT MATTER

IPC 6   G01N27/64

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 6   G01N

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 5 234 838 A (BACON JR ALLAN T) 10 August 1993	1-3, 7-10,13
Y	see abstract	5,6,11, 12
	see column 1, line 22 - line 53 see column 2, line 40 - line 51 see column 4, line 13 - line 49 see column 4, last paragraph; claim 1; figure 1	

Y	WO 93 11554 A (GRASEBY DYNAMICS LTD) 10 June 1993 cited in the application see abstract; claim 3	11,12

	-/--	

[X] Further documents are listed in the continuation of box C.   [X] Patent family members are listed in annex.

* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&" document member of the same patent family

Date of the actual completion of the international search	Date of mailing of the international search report
29 April 1997	0 9. 05. 97

Name and mailing address of the ISA	Authorized officer
European Patent Office, P.B. 5818 Patentlaan 2 NL - 2280 HV Rijswijk Tel.: (+ 31-70) 340-2040, Tx. 31 651 epo nl, Fax: (+ 31-70) 340-3016	Hulne, S

Form PCT/ISA/210 (second sheet) (July 1992)

1

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	ANALYTICAL CHEMISTRY, vol. 56, 1984, COLUMBUS US, pages 1794-1797, XP002030473 C. J. PROCTOR: "Alternative Reagent ions for plasma chromatography." cited in the application see abstract see page 1794, right-hand column, paragraph 3	5,6
A	US 5 095 206 A (BACON JR ALLAN T ET AL) 10 March 1992 see abstract; claim 1; figure 1	1

1

Patent document cited in search report	Publication date	Patent family member(s)		Publication date
US 5234838 A	10-08-93	US	5032721 A	16-07-91
		US	5283199 A	01-02-94
		US	5095206 A	10-03-92
WO 9311554 A	10-06-93	EP	0615655 A	21-09-94
		IL	103963 A	31-03-96
		JP	7502143 T	02-03-95
US 5095206 A	10-03-92	US	5032721 A	16-07-91
		AT	134069 T	15-02-96
		CA	2043708 A	02-12-91
		DE	69117045 D	21-03-96
		DE	69117045 T	19-09-96
		EP	0509171 A	21-10-92
		US	5283199 A	01-02-94
		US	5234838 A	10-08-93